SIEMENS

UROSKOP D2 / D3

SP

Service Information

Splash Protection for II 33/40

© Siemens AG 1996
The reproduction, transmission or use of this document or its contents is not permitted without express written authority. Offenders will be liable for damages. All rights, including rights created by patent grant or registration of a utility model or design, are reserved.

English
Print No.: RLL5-310.076.05.01.02
Doc.generation Date: 06.96
Replaces: n.a.

Splash Protection for II 33/40

Material

1 Splash protection:	Part no.: 72 96 171 G5178
1 Punched rubber band:	Part no.: 45 38 963 EH725
1 Adhesive tape:	Part no.: 34 74 988
2 Washers:	Part no.: 33 86 919
1 Screw M4 x 10	
1 Nut M4	

Tools

- Service tool set
- Scissors

Installation

- Unscrew the cover panels around the II mounting flange (underneath the table).
- Place the splash protection around the image intensifier housing according to the drawing and secure its upper rim with adhesive tape.
  Make sure the foil covers the II smoothly and without wrinkling, with the ends overlapping on the rear part. It might be helpful to use short strips of adhesive tape for preliminary attachment of the splash protection before attaching the final strip of tape.
- Lay the punched rubber band tightly around the splash protection foil attached to the image intensifier.
- Use the supplied screw and nut with the two washers to join both ends of the punched rubber band.
- Cut off the excessive length of the rubber band as required (see drawing).
- Reinstall the cover panels around the II mounting flange.

Splash Protection for II 33/40

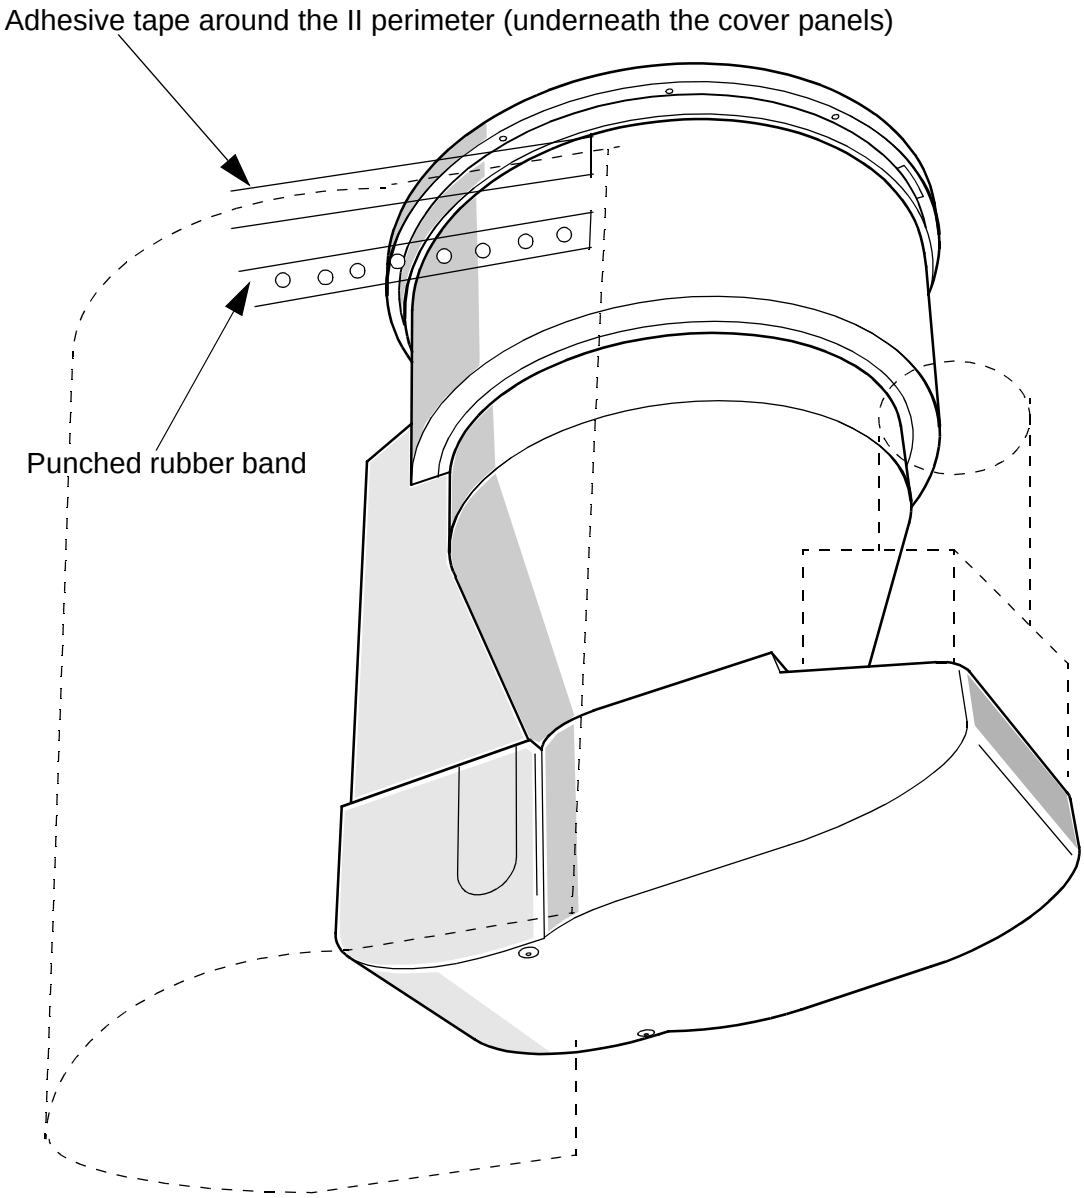

TD SP 2 / Sauter
TD SP 1 / Schlee
AUT 98 / Dr. McMinn

This page intentionally left blank.